

A photograph of a multi-channel pipette with several tips, each containing a small amount of purple liquid. The pipette is positioned over a clear microplate. In the background, a laboratory setting is visible with a rack of test tubes, some containing orange liquid, and a petri dish in the foreground. The image is overlaid with a semi-transparent white circle.

IL-10 (pig)

For laboratory research only. Not for human or veterinary diagnostic use.

Bertin Bioreagent also markets pre-analytical products, EIA kits, antibodies & biochemicals for:

- ▶ **Inflammation**
- ▶ **Oxidative injury**
- ▶ **Endocrinology**
- ▶ **Diabetes**
- ▶ **Obesity**
- ▶ **Hypertension**
- ▶ **Pain**
- ▶ **Prion diseases**

Do not hesitate to contact our after-sales services for further information at tech@bertin-bioreagent.com

IL-10 (pig)
ELISA kit
#A05414.96 wells

For research laboratory use only
Not for human diagnostic use

This assay was developed
& validated by Bertin Bioreagent

Fabriqué en France
Made in France



#A11414
Version: 0118

Table of contents

▶ PRECAUTION FOR USE.....	6
▶ BACKGROUND.....	7
▶ PRINCIPLE OF THE ASSAY	8
▶ ASSAY CHARACTERISTICS	10
▶ MATERIALS AND EQUIPMENT REQUIRED.....	10
▶ SAMPLE COLLECTION AND PREPARATION.....	11
▶ REAGENT PREPARATION	12
▶ ASSAY PROCEDURE	14
▶ ASSAY PROCEDURE SUMMARY	19
▶ DATA ANALYSIS.....	19
▶ ACCEPTABLE RANGE.....	20
▶ TYPICAL RESULTS.....	21
▶ TROUBLESHOOTING	22
▶ BIBLIOGRAPHY	23

96 wells**Storage: +4°C****Expiry date: stated on the package**

This kit contains:

Designation	Colour of cap	Item #	Quantity per kit	Form
IL-10 precoated 96-well Strip Plate	Blister with zip	A08414.1 ea	1	-
Streptavidin Poly_HRP Tracer	Green	A04410.100 dtn	1	Liquid
IL-10 (pig) Biotin-labelled Antibody	Red	A03414.100 dtn	1	Liquid
IL-10 (pig) Standard	Blue with red septum	A06414.1 ea	2	Lyophilised
Poly_HRP EIA Buffer	Grey / Blue	A07410.1 ea	1	Lyophilised
Wash Buffer	Silver	A17000.1 ea	1	Liquid
Tween 20	Transparent	A12000.1 ea	1	Liquid
HRP Substrate Solution	Black	A09034.100 dtn	1	Liquid
HRP Stop Solution	Yellow	A22410.100 dtn	1	Liquid
Technical Booklet	-	A11414.1 ea	1	-
Well cover Sheet	-	-	1	-

Each kit contains sufficient reagents for 96 wells. This allows for the construction of one standard curve in duplicate and the assay of 37 samples in duplicate.

► **Precaution for use**

Users are recommended to carefully read all instructions for use before starting work.

Each time a new pipette tip is used, aspirate a sample or reagent and expel it back into the same vessel. Repeat this operation two or three times before distribution in order to equilibrate the pipette tip.

- For research laboratory use only
- Not for human diagnostic use
- Do not pipet liquids by mouth
- Do not use kit components beyond the expiration date
- Do not eat, drink or smoke in area where kit reagents are handled
- Avoid splashing

HRP Stop Solution and HRP Substrate Solution are harmful solutions. To avoid any contact, wear eye, hand, face and clothing protection when handling these.

Wearing gloves, laboratory coat and glasses is recommended when assaying kit materials and samples.

► **Temperature**

Unless otherwise specified, all the experiments are done at room temperature (RT), which is around +20°C. Working at +25°C or more affects the assay and decreases its efficiency.

► Background

Also known as cytokine synthesis inhibitory factor (CSIF), IL-10 is a glycosylated polypeptide of 157 amino acids [1,2]. The mature IL-10 is a homodimer linked by two intrachain disulphide bridges [3] (each sub-unit is 157 aa).

IL-10 is produced by innate and non-innate cells, it is a cytokine of the innate and adaptive immunity. The mammalian cells known to secrete IL-10 are NK cells [4], cytotoxic T cells, memory Th1 and Th2 cells [5], macrophages, monocytes, B cells, dendritic cells, hepatic stellates, keratinocytes [6] and fetal erythroblasts [7].

IL-10 is a cytokine with multiple pleiotropic effects in immunoregulation and inflammation. IL-10 is characterized as an anti-inflammatory cytokine: it represses the expression of inflammatory cytokines, such as Tumor Necrosis Factor-alpha (TNF-alpha), Interleukin-6 (IL-6) and Interleukin-1 (IL-1 beta), in macrophages [8, 9]. IL-10 is an immunoregulation cytokine: it negatively regulates Th1 responses by downmodulating antigen presenting capacity of APC.

Due to its central function, a dysregulation of the IL-10 production is implicated in asthma or autoimmune diseases. IL-10 is currently studied in immuno-oncology.

► **Principle of the assay**

The enzymatic immunoassay (EIA/ELISA) is based on a sandwich technique. Wells of supplied plate are coated with a polyclonal antibody specific to IL-10 (pig).

IL-10 (pig) introduced into the wells (standard or sample) is bound by the polyclonal antibody coated on the plate and is then detected by another polyclonal antibody tagged with biotin also specific of IL-10 (pig).

The two antibodies then form a sandwich by binding on different epitopes of the IL-10 (pig).


The sandwich is immobilised on the plate where excess reagents are washed away.

The immunological complex is revealed by the interaction between biotin and streptavidin labelled with HRP (Tracer).

The concentration of IL-10 (pig) is determined by measuring the enzymatic activity of immobilized Tracer using TMB. The Tracer acts on TMB to form a yellow compound after the reaction has been stopped.

The intensity of the colour, which is determined by spectrophotometry at 450 nm, is proportional to the amount of IL-10 (pig) present in the well during the immunological incubation.

The principle of the assay is summarised below:

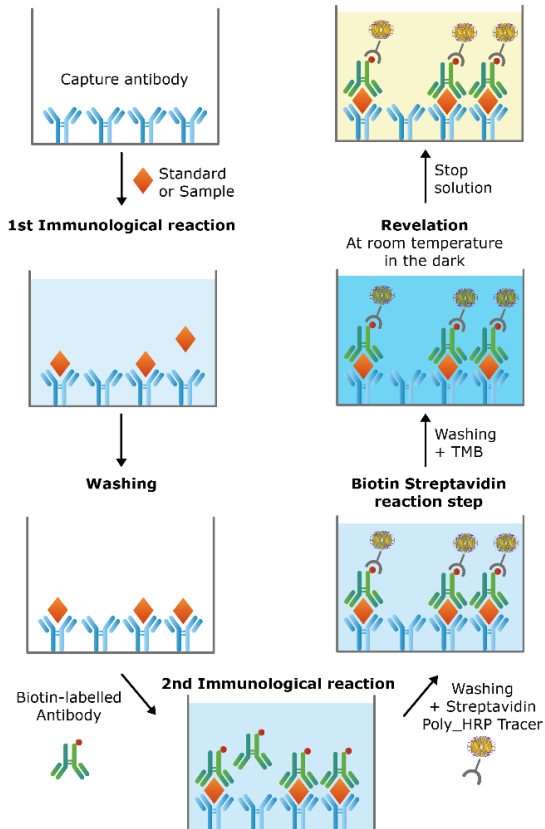

► Assay characteristics

All data shown below are from experiments realized in buffer.

- > **Limit of detection (LOD):** ≤ 0.16 ng/mL (calculated as the concentration of IL-10 (pig) corresponding to the NSB average plus three standard deviations)
- > **Cross-reactivity**

Molecule/Species	Cross-reactivity
Recombinant IL-10 (bovine)	None
Recombinant IL-10 (mouse)	None

► Materials and equipment required

In addition to standard laboratory equipment, the following materials are required.

For the assay:

- Precision micropipettes (20 to 1000 μ L)
- Spectrophotometer plate reader (450 nm filter)
- Microplate washer (or wash bottles)
- Orbital microplate shaker
- Multichannel pipette and disposable tips 30-300 μ L
- UltraPure water #A07001.1L
- Polypropylene tubes

Water used to prepare all ELISA reagents and buffers must be UltraPure (deionized & free from organic contaminant traces).



Do not use distilled water, HPLC-grade water or sterile water.

- UltraPure water may be purchased from Bertin Bioreagent (item #A07001.1L).

▶ **Sample collection and preparation**

This assay may be used to measure IL-10 (pig).



It is the responsibility of the user to check the compatibility of the assay with the study matrix.

▶ **General precautions**

- All samples must be free from organic solvents prior to assay.
- Samples should be assayed immediately after collection or should be stored at -20°C or at -80°C.

► Reagent preparation

Each kit contains sufficient reagents for 96 wells. This allows for the construction of one standard curve in duplicate and the assay of 37 samples in duplicate.

An additional vial of Standard is provided in case you need to perform 2 assays with the kit.

All reagents must be brought to room temperature (around +20°C) prior to use the assay.

► Poly_HRP EIA Buffer

Reconstitute the Poly_HRP EIA Buffer #A07410 with 25 mL of UltraPure water. Allow it to stand 5 minutes until completely dissolved and then mix thoroughly by gentle inversion.

Stability at 4°C: 1 month.



Before use, filter the Buffer on 0.22 µm filter.

► IL-10 (pig) Standard

Reconstitute the IL-10 (pig) Standard vial #A06414 with 1 mL of UltraPure water. Allow it to stand for 5 minutes until completely dissolved and then mix thoroughly by gentle inversion.

The concentration of the first standard (S1) is 10 ng/mL. Prepare seven polypropylene tubes (for the seven other standards) and add 500 µL of Poly_HRP EIA Buffer into each

tube. Then prepare the standards by serial dilutions as follow:

Standard	Volume of Standard	Volume of Poly_HRP EIA Buffer	Standard concentration
S1	-	-	10.00ng/mL
S2	500 μ L of S1	500 μ L	5.00ng/mL
S3	500 μ L of S2	500 μ L	2.50ng/mL
S4	500 μ L of S3	500 μ L	1.25ng/mL
S5	500 μ L of S4	500 μ L	0.62ng/mL
S6	500 μ L of S5	500 μ L	0.31ng/mL
S7	500 μ L of S6	500 μ L	0.16ng/mL
S8	500 μ L of S7	500 μ L	0.08ng/mL

Stability at 4°C: within the day

▶ **IL-10 (pig) Biotin-labelled Antibody**

Supplied IL-10 (pig) Biotin-labelled Antibody is concentrated 10 times. Calculate the volume needed (number of wells multiplied by 0.1 mL) and then dilute the IL-10 (pig) Biotin-labelled Antibody solution #A03414 with the appropriate volume of Poly_HRP EIA Buffer.

Example: for 40 wells you need 4 mL of IL-10 (pig) Biotin-labelled Antibody (40 x 0.1 mL), add 0.4 mL of IL-10 (pig) Biotin-labelled Antibody in 3.6 mL of Poly_HRP EIA Buffer.

Stability of diluted antibody at +4°C: within the day.

▷ **Wash Buffer**

Dilute 2 mL of concentrated Wash Buffer #A17000 with 800 mL of UltraPure water. Add 400 μ L of Tween 20 #A12000. Use a magnetic stirring bar to mix the content.

Stability at +4°C: 1 month.

▶ **Assay procedure**

It is recommended to measure the samples in duplicate following the instruction below.

▷ **Plate preparation**

Prepare the Wash Buffer as indicated in the reagent preparation section.

Open the plate pouch and select enough strips for your assay. Place unused strips back in the pouch.

Stability at +4°C: 1 month.

Rinse each well 5 times with Wash Buffer (300 μ L/well).

Just before distributing the reagents and samples, remove the buffer from the wells by inverting the plate and blot the last drops by tapping it on paper towels.

▶ **Plate set-up**

A plate set-up is suggested hereafter. The contents of each well may be recorded on the template sheet provided at the end of this technical booklet.

	1	2	3	4	5	6	7	8	9	10	11	12
A	Bk	S7	S3	*	*	*	*	*	*	*	*	*
B	Bk	S7	S3	*	*	*	*	*	*	*	*	*
C	Bk	S6	S2	*	*	*	*	*	*	*	*	*
D	NSB	S6	S2	*	*	*	*	*	*	*	*	*
E	NSB	S5	S1	*	*	*	*	*	*	*	*	*
F	NSB	S5	S1	*	*	*	*	*	*	*	*	*
G	S8	S4	*	*	*	*	*	*	*	*	*	*
H	S8	S4	*	*	*	*	*	*	*	*	*	*

Bk : Blank

S1-S8 : Standards 1-8

NSB : Non Specific Binding

* : Samples or Quality Controls

▶ **Pipetting the reagents**

Samples and reagents must reach room temperature prior performing the assay.

Use new tips to pipet buffers, standards, samples, antibody and other reagents.

Before pipetting, equilibrate the pipette tips in each reagent. Do not touch the liquid already in the well when expelling with the pipette tip.

> ***Poly_HRP EIA Buffer***

Dispense 100 μ L to Non Specific Binding wells (NSB) wells.

> ***IL-10 (pig) Standard***

Dispense 100 μ L of each of the eight standards (S8 to S1) in duplicate to appropriate wells.

Start with the lowest concentration standard (S8) and equilibrate the tip in the next higher standard before pipetting.

> ***Sample***

Dispense 100 μ L in duplicate to appropriate wells. Highly concentrated samples may be diluted in Poly_HRP EIA Buffer.

▷ **Incubating the plate**

Cover the plate with cover sheet and incubate 120 minutes at room temperature, shaking at 300 rpm on an orbital microplate shaker.

▷ **Washing the plate**

Rinse each well 5 times with Wash Buffer (300 µL/well). Just before distributing reagents, remove the buffer from the wells by inverting the plate and shaking out the last drops on a paper towel.

▷ **Pipetting the reagents**

> ***IL-10 (pig) Biotin-labelled antibody***

Dispense 100 µL to each well, except Blank (Bk) wells.

▷ **Incubating the plate**

Cover the plate with the cover sheet and incubate 60 minutes at room temperature, shaking at 300 rpm on an orbital microplate shaker.

▷ **Washing the plate**

Rinse each well 5 times with Wash Buffer (300 µL/well). Just before distributing reagents, remove the buffer from the wells by inverting the plate and shaking out the last drops on a paper towel.

▷ **Pipetting the reagents**

> ***Streptavidin Poly_HRP Tracer***

Dispense 100 µL to each well, except Blank (Bk) wells.

▷ **Incubating the plate**

Cover the plate with the cover sheet and incubate 30 minutes at room temperature, shaking at 300 rpm on an orbital microplate shaker.

▷ **Developing and reading the plate**

- Empty the plate by turning it over. Rinse each well 5 times with 300 μ L of Wash Buffer. At the end of the last washing step, empty the plate and blot the plate on a paper towel to discard any trace of liquid.
- Add 100 μ L of HRP Substrate Solution to each well.
- Incubate the plate in the dark at room temperature without shaking. For the time, look at the lot specific Quality Control Sheet (QCS). In general, revelation time is 10 min.
- Add 100 μ L of HRP Stop Solution to each well.
- Wipe the bottom of the plate with a paper towel, and make sure that no liquid has splashed outside the wells.
- Read the plate at 450 nm (yellow color).

► Assay procedure summary

Enzyme Immunoassay Protocol (volumes are in μL)				
	Blank	NSB	Standard	Sample
Poly_HRP EIA Buffer	-	100	-	-
Standard	-	-	100	-
Sample	-	-	-	100
Cover plate, incubate 120 minutes at room temperature under orbital shaking at 300 rpm				
Wash strips 5 times with 300 μL /well Discard liquid from the wells & dry on absorbent paper				
Biotin-labelled Antibody	-	100		
Cover plate, incubate 60 minutes at room temperature under orbital shaking at 300 rpm				
Wash strips 5 times with 300 μL /well Discard liquid from the wells & dry on absorbent paper				
Streptavidin Poly_HRP Tracer	-	100		
Cover plate, incubate 30 minutes at room temperature under orbital shaking at 300 rpm				
Wash strips 5 times with 300 μL /well Discard liquid from the wells & dry on absorbent paper				
HRP Substrate Solution	100			
Incubate the plate in the dark without agitation				
HRP Stop Solution	100			
Read the plate at 450 nm				

► Data analysis

Make sure that your plate reader has subtracted the absorbance readings of the blank wells from the absorbance readings of the rest of the plate. If it is not the case, please do it at this step.

- Calculate the average absorbance for each NSB, standard and sample.
- For each standard, plot the absorbance on y axis versus the concentration on x axis. Draw a best-fit line through the points.

- To determine the concentration of your samples, find the absorbance value of each sample on the y axis.
- Read the corresponding value on the x axis which is the concentration of your unknown sample.
- Samples with a concentration greater than 10 ng/mL should be re-assayed after dilution in Poly_HRP EIA Buffer.
- Most plate readers are supplied with a curve-fitting software capable of graphing these data (4-parameter logistic fit 4PL). If you have this type of software, we recommend using it. Refer to it for further information.

▶ **Acceptable range**

- NSB absorbance ≤ 0.06 A.U.
- Limit of detection ≤ 0.16 μ UI/mL


► Typical results

The following data are for demonstration purpose only. Your data may be different and still correct.

These data were obtained using all reagents as supplied in this kit under the following conditions: 10 minutes developing at room temperature, reading at 450 nm. A 4 parameter logistic fitting was used to determine the concentrations.

Standard	IL-10 (pig) ng/mL	Absorbance A.U.
S1	10.00	1.067
S2	5.00	0.586
S3	2.50	0.320
S4	1.25	0.172
S5	0.62	0.099
S6	0.31	0.059
S7	0.16	0.039
S8	0.08	0.029
NSB	0.00	0.021

Typical IL-10 (pig) standard curve

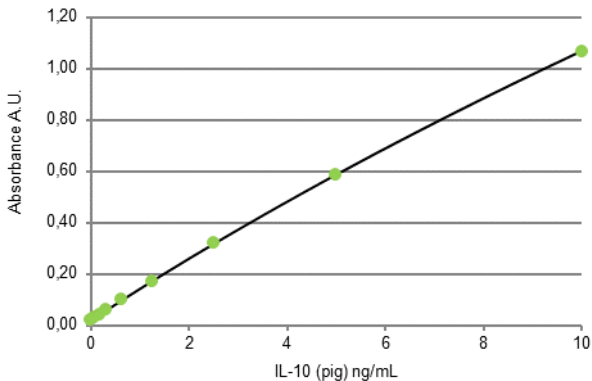

► Troubleshooting

> ***Absorbance values are too low:***

- one of the reagents was not properly dispensed,
- incorrect preparation,
- assay performed before reagents reached room temperature,
- reading time not long enough.

> **High signal and background in all wells:**

- inefficient washing,
- overdeveloping (incubation time should be reduced),
- high ambient temperature.

> **High dispersion of duplicates:**

- poor pipetting
- irregular plate washing.

These are a few examples of troubleshooting that may occur. If further information or explanation is needed, please contact Bertin Bioreagent Technical Support by phone on +33 (0)139 306 036, fax +33 (0)139 306 299 or by E-mail tech@bertin-bioreagent.com. Please have batch number of the kit (see outside the box) ready to provide to the technical support.

Bertin Bioreagent offers EIA Training kit #B05005. Feel free to contact our Technical Support. We are always happy to hearing from you.

► **Bibliography**

1. Blancho G., Gianello P., Germana S. et al
Molecular identification of porcine interleukin 10: regulation of expression in a kidney allograft model.

Proc Natl Acad Sci USA 1995 Mar 28;92(7):2800-4.

2. Moore K.W., de Waal Malefyt R., Coffman R.L. et al
Interleukin-10 and the interleukin-10 receptor

Annu Rev Immunol. 2001;19:683-765.

- 3.** Windsor W.T., Syto R., Tsarbopoulos A. et al
Disulfide bond assignments and secondary structure analysis of human and murine interleukin 10.
Biochemistry. 1993 Aug 31;32(34):8807-15.
- 4.** Mehrotra P.T., Donnelly R.P., Wong S. et al
Production of IL-10 by human natural killer cells stimulated with IL-2 and/or IL-12.
J Immunol. 1998 Mar 15;160(6):2637-44.
- 5.** Yssel H., De Waal Malefyt R., Roncarolo M.G. et al
IL-10 is produced by subsets of human CD4+ T cell clones and peripheral blood T cells.
J Immunol. 1992 Oct 1;149(7):2378-84.
- 6.** Grewe M., Gyufko K., Krutmann J.
Interleukin-10 production by cultured human keratinocytes: regulation by ultraviolet B and ultraviolet A1 radiation.
J Invest Dermatol. 1995 Jan;104(1):3-6.
- 7.** Sennikov S.V., Krysov S.V., Silkov A.N.
Production of IL-10, TNF-alpha, IFN-gamma, TGF-beta by different populations of erythroid cells derived from human embryonal liver.
Cytokine. 2002 Feb 21;17(4):221-5.
- 8.** Williams L.M., Ricchetti G., Sarma U. et al
Interleukin-10 suppression of myeloid cell activation - a continuing puzzle.
Immunology 2004 Nov;113(3):281-92
- 9.** Hu X., Chen J., Wang L. et al
Crosstalk among Jak-STAT, Toll-like receptor, and ITAMdependent pathways in macrophage activation.
Journal of leukocyte biology 2007 Aug;82(2):237-43

With 30 years of experience, Bertin Bioreagent develops and sells best-in-class kits and products for life science research labs. Our scientist team innovate each day to tailor biomarker assays, pre-analytical products, kits, antibodies and biochemicals that are ready to use, fully validated with a strict quality control.

We strive to address a broad range of research interest: inflammation, oxidative injury, endocrinology, diabetes, obesity, hypertension, pain, prion diseases.

Bertin Bioreagent has also a long expertise in developing customized solutions adapted to your need. Feel free to contact us for your special projects!

To offer a complete solution to researchers, Bertin Instruments offers a range of unique laboratory equipment from Air Sample collection, Sample Homogenisation and Digital Imaging.

Our products are available worldwide through us directly or via our distributor network. Our sales team is active on all continents and will be delighted to answer all your commercial questions.

Should you need help with a product, you can contact our technical support by emailing to tech@bertin-bioreagent.com

Should you need help with an order, you can contact our customer service by emailing to order@bertin-bioreagent.com

Please visit our websites:
Bertin-instruments.com
Bertin-Bioreagent.com
Bertin-Corp.com



CONTACT US

Bertin Technologies
10 bis Avenue Ampère
Parc d'Activités du Pas du Lac
78180 Montigny-le-Bretonneux
FRANCE



+33 (0)139 306 036



tech@bertin-bioreagent.com



EU webstore: Bertin-bioreagent.com
US webstore: Bertin-corp.com